

FIG. 1

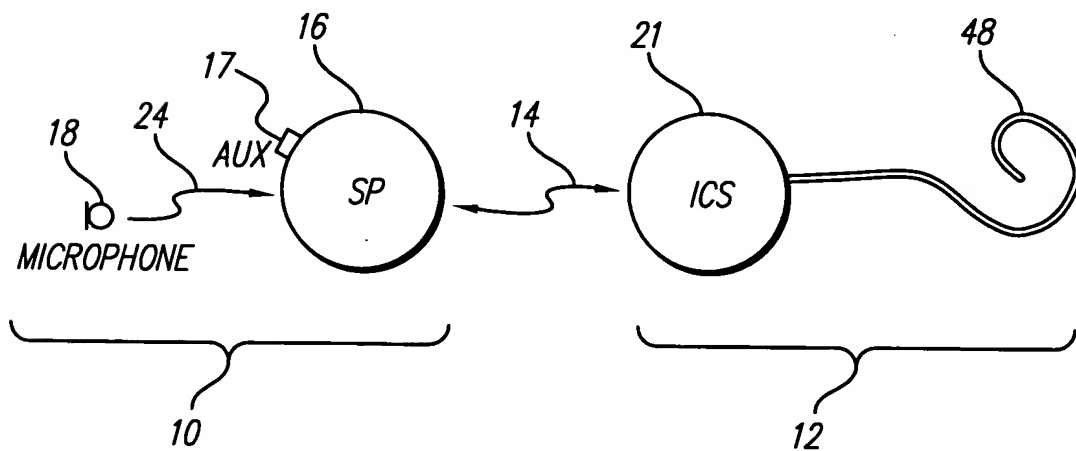


FIG. 2A

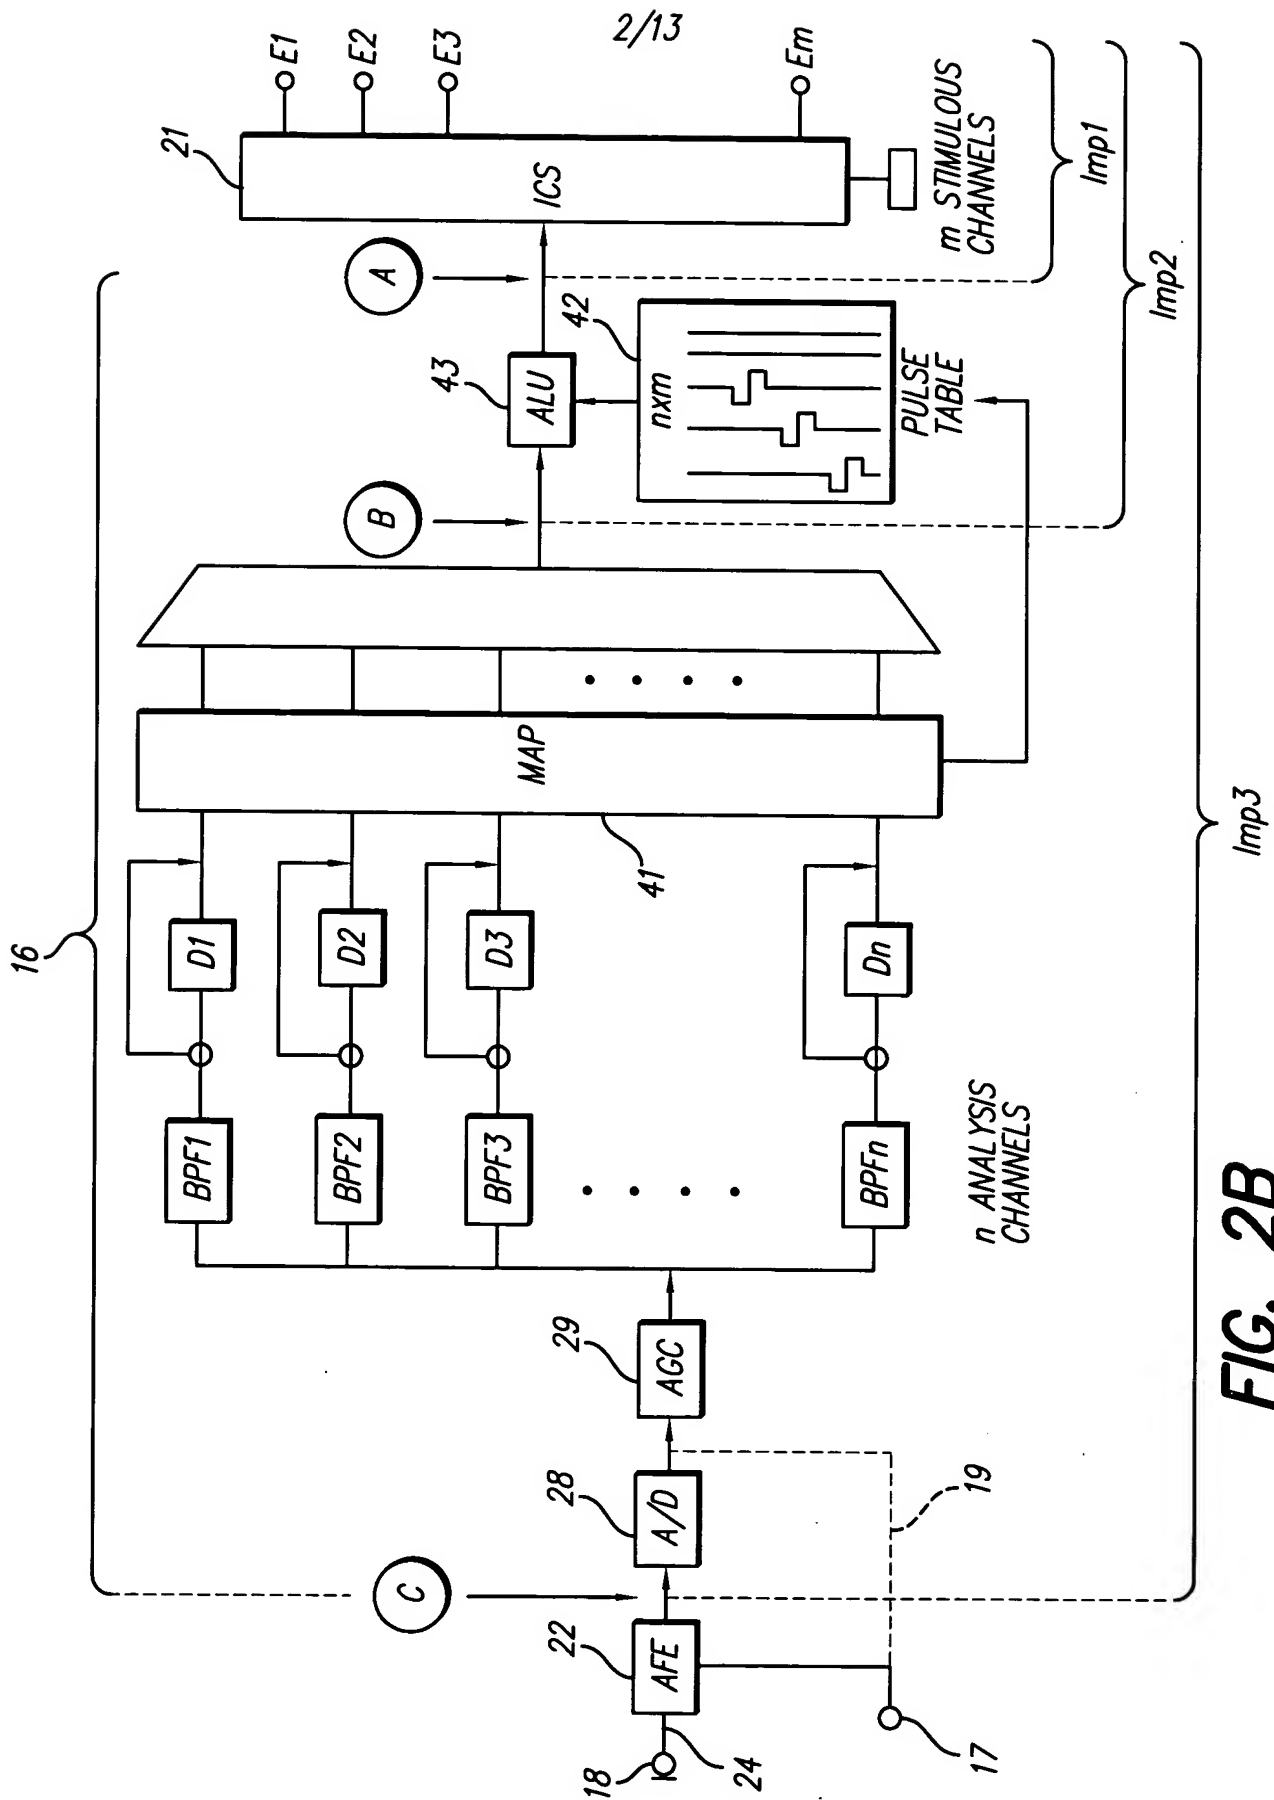
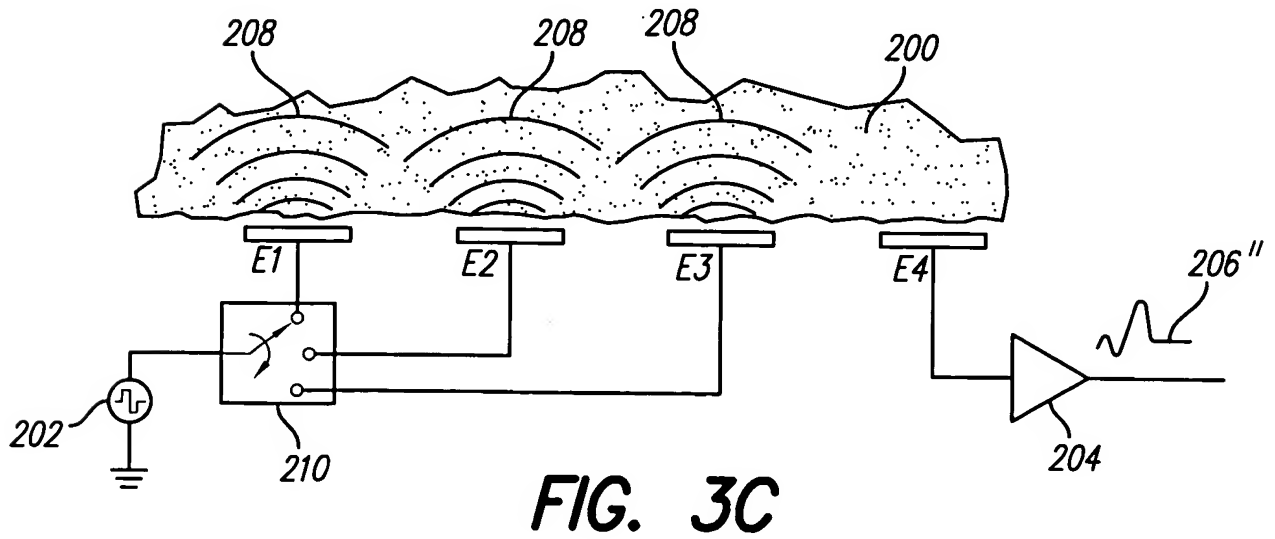
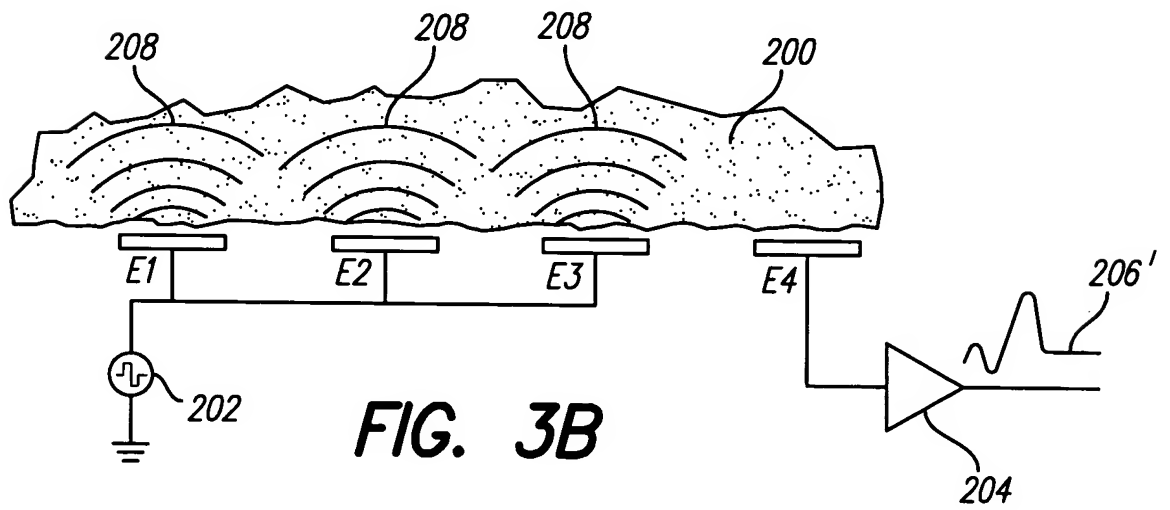
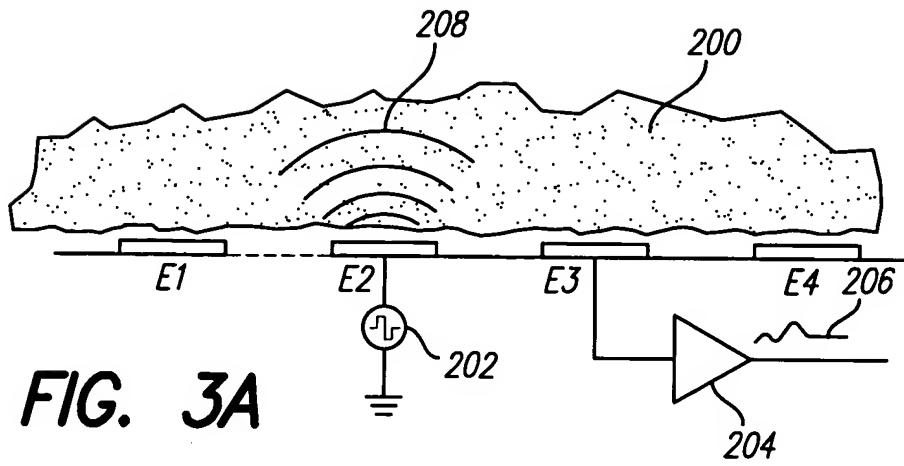


FIG. 2B



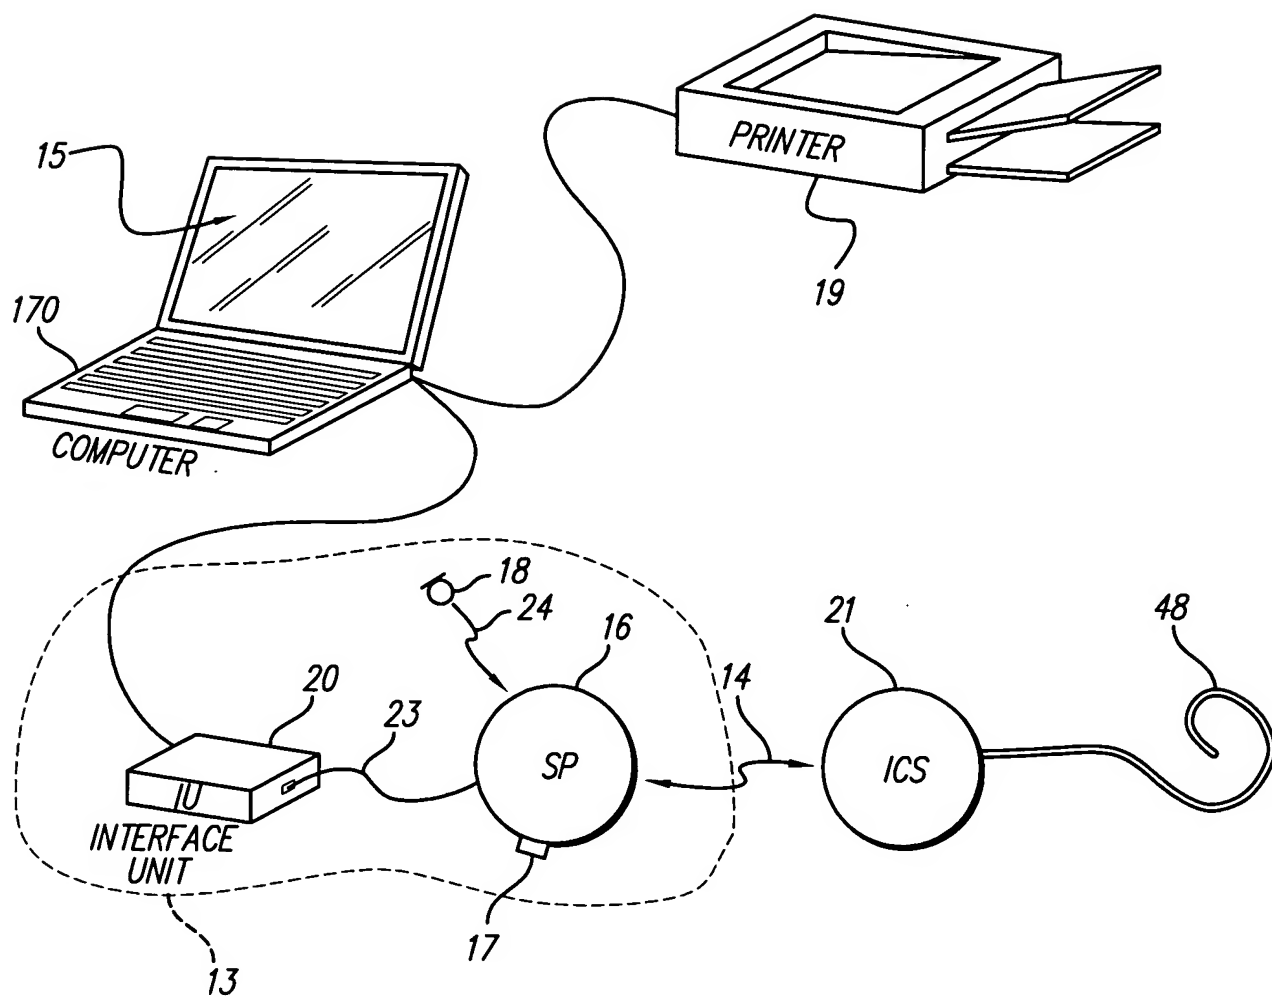


FIG. 4A

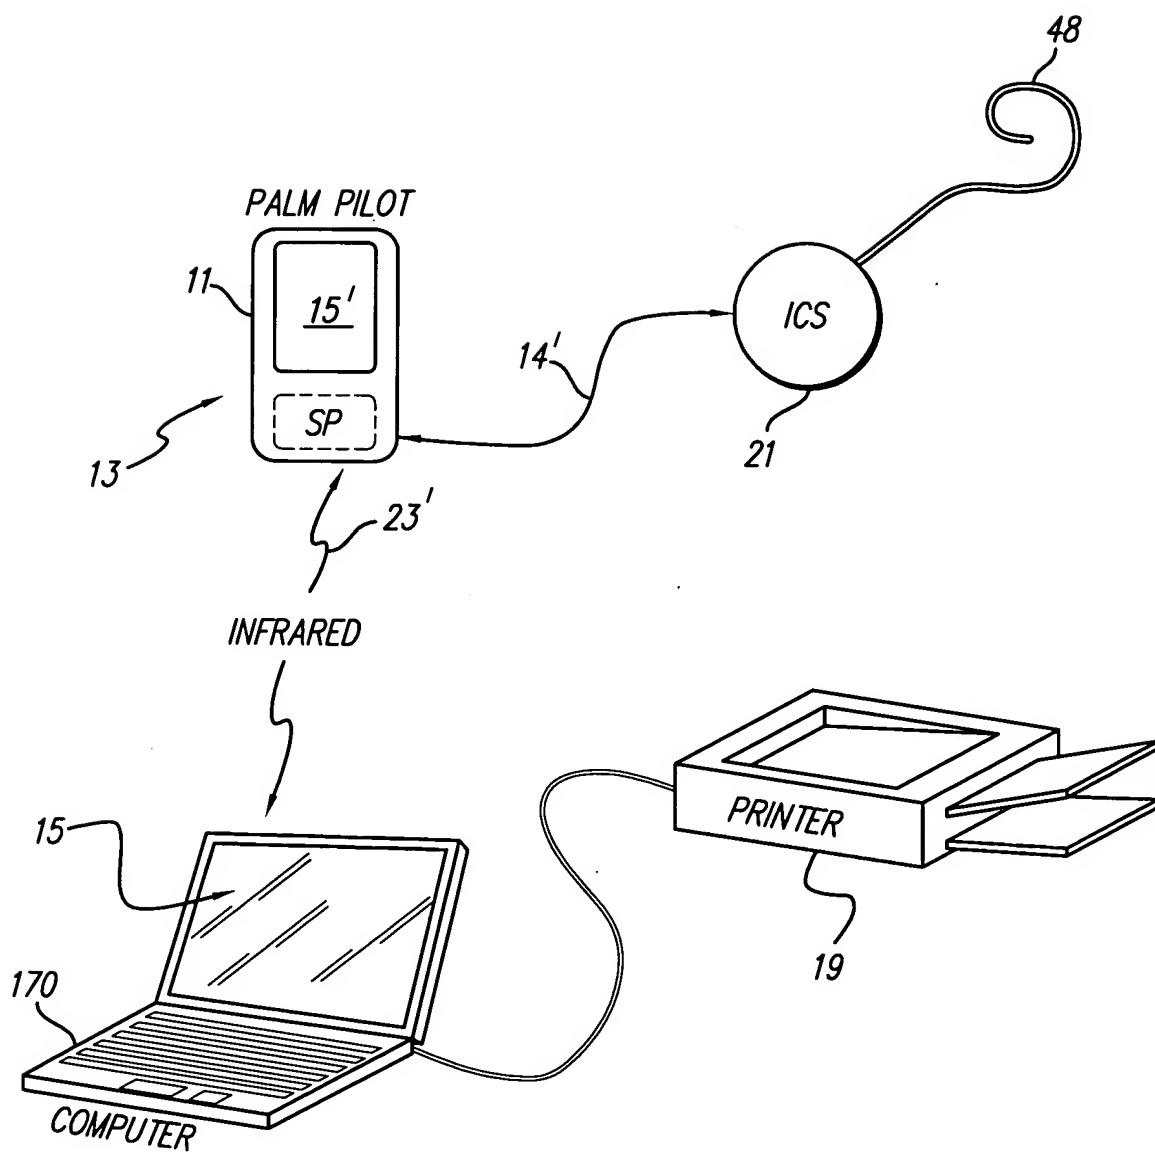
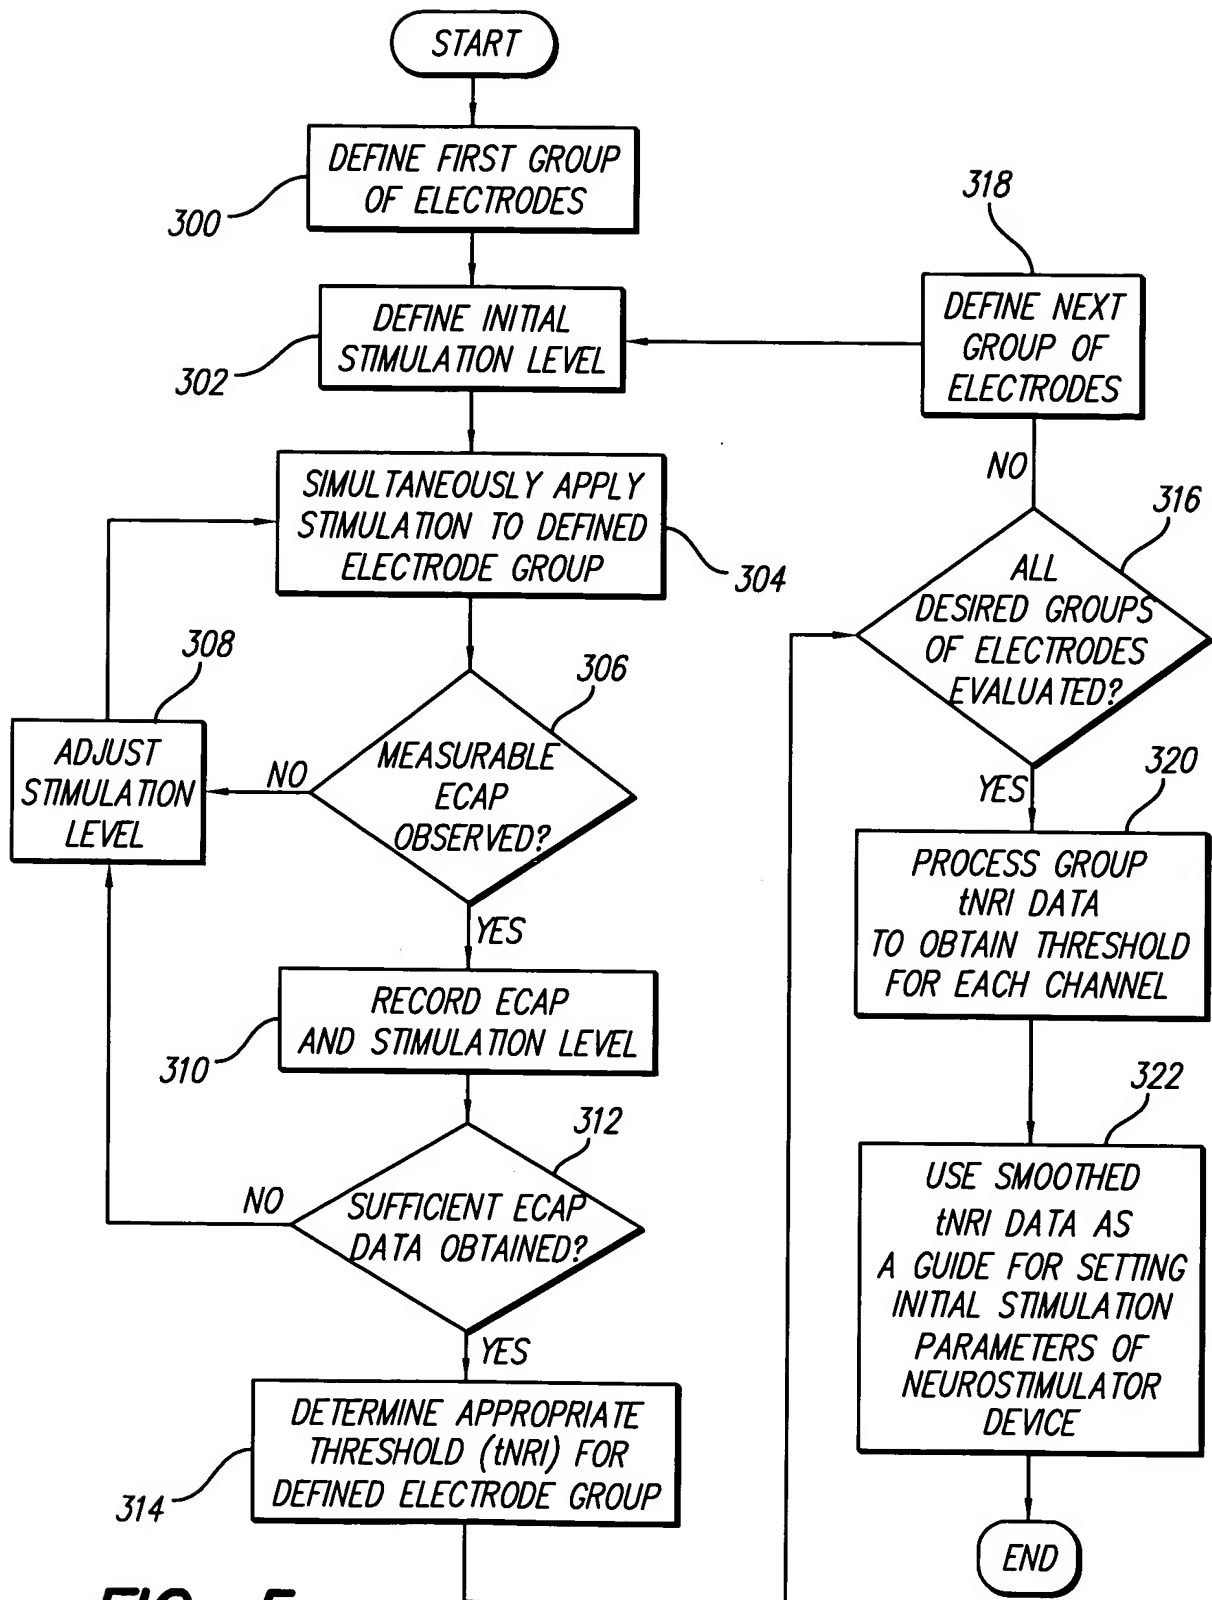


FIG. 4B

**FIG. 5**

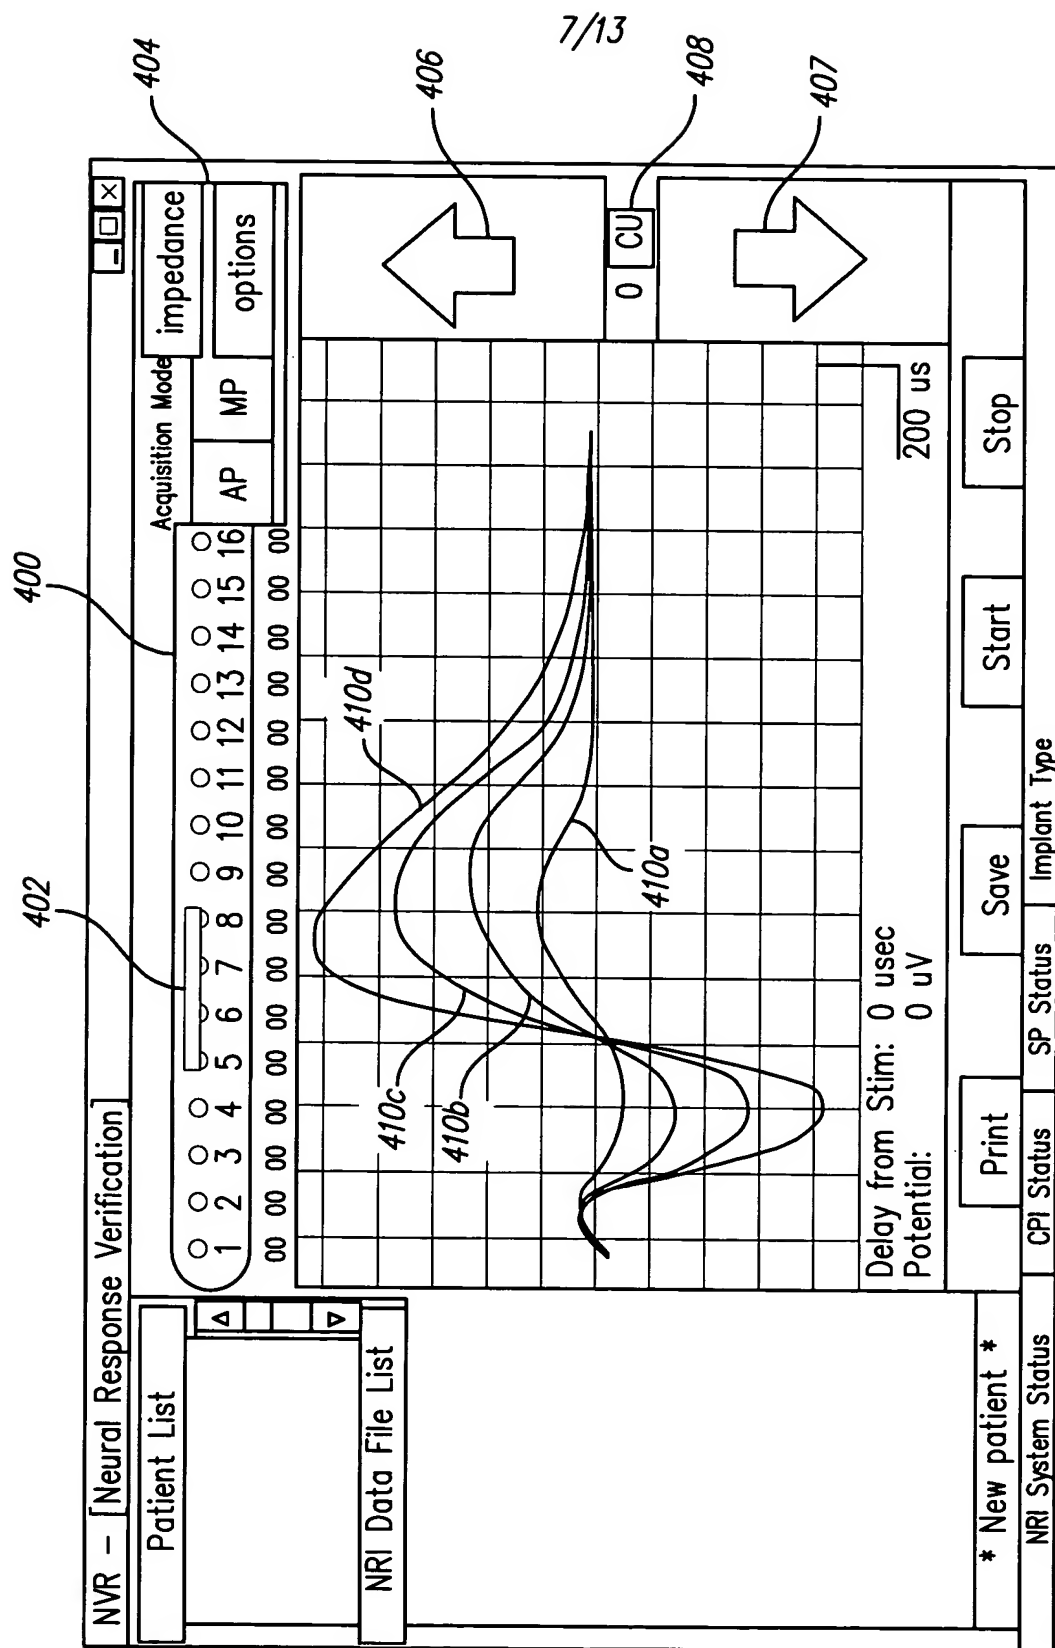


FIG. 6A

NVR - Neural Response Verification
404

Patient List

NRI Data File List

12345678910111213141516

00000000000000000000000000000000

Manual plot

Grouping

OK

Macro

Defaults

CANCEL

Delay from Stim: 0 usec

200 us

Potential: 0 uV

0 CU

impedance

options

↑

0 CU

↓

Stop

Start

Save

Print

* New patient *

NRI System Status

CPI Status

SP Status

Implant Type

FIG. 6B

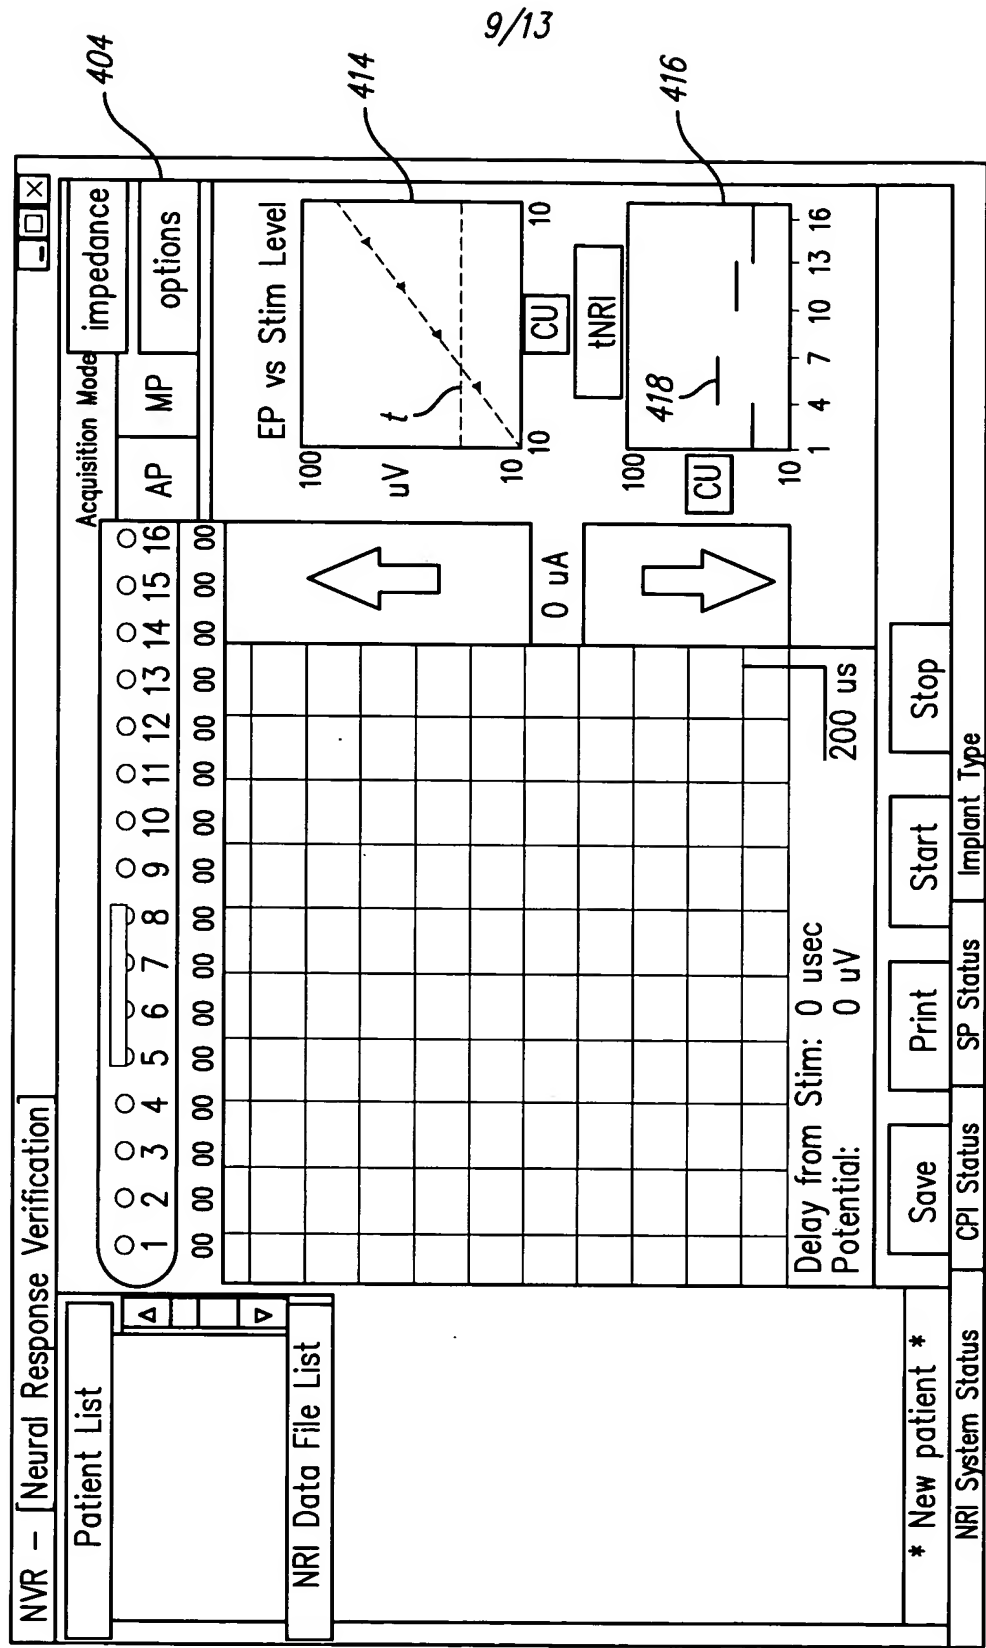


FIG. 6C

426-

FIG. 6E

FIG. 6F

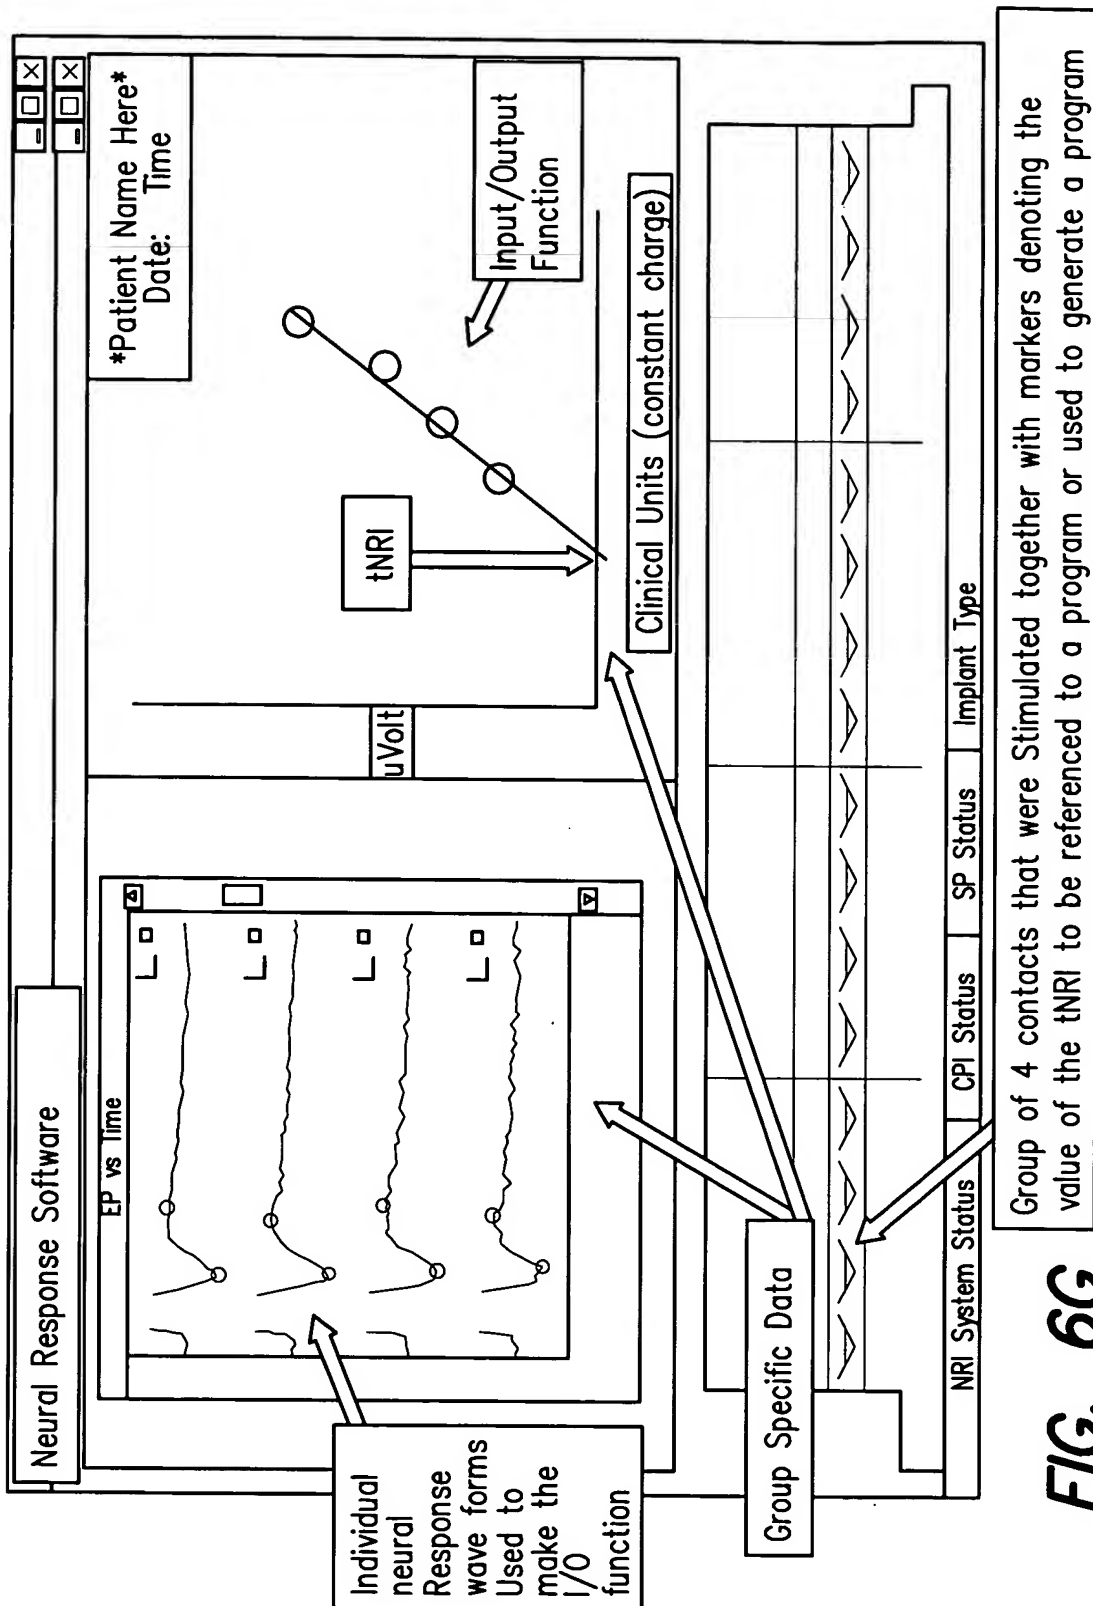


FIG. 6G